

Article

Performance of PEth Compared With Other Alcohol Biomarkers in Subjects Presenting For Occupational and Pre-Employment Medical **Examination**

Jasna Neumann¹, Olof Beck^{1,2}, Anders Helander^{0,3}, and Michael Böttcher^{1,*}

¹MVZ Labor Dessau GmbH, Bauhüttenstrasse 6, D-06847 Dessau-Roßlau, Germany, ²Department of Clinical Neuroscience, CPF, Norra Stationsgatan 69, Karolinska Institutet, Stockholm, SE-171 77, Sweden, and ³Department of Laboratory Medicine, C1:74, Karolinska University Hospital, Karolinska Institutet, Stockholm, SE-141 86, Sweden

*Corresponding author: MVZ Labor Dessau GmbH, Bauhüttenstrasse 6, D-06847 Dessau-Roßlau, Germany.

Tel.: +493405405372; Fax: +493405405376; E-mail: michael.boettcher@laborpraxis-dessau.de

Received 18 January 2020; Revised 14 March 2020; Editorial Decision 24 March 2020; Accepted 24 March 2020

Abstract

Aims: To compare the performance of short- and long-term alcohol biomarkers for the evaluation of alcohol drinking in employment-related health controls.

Methods: The 519 blood samples originated from 509 patients (80% men) presenting at occupational health units and medical centers at employment agencies for the evaluation of risky drinking. The laboratory investigation comprised the measurement of phosphatidylethanol (PEth 16:0/18:1), carbohydrate-deficient transferrin (CDT; % disialotransferrin), gamma-glutamyl transferase (GGT), mean corpuscular volume (MCV), ethanol and ethyl glucuronide (EtG).

Results: Many samples tested positive for acute (57%) and chronic (69%) alcohol biomarkers. PEth was the single most positive biomarker (64%; cut-off 0.05 µmol/l or 35 µg/l) and the only positive chronic biomarker in 100 cases. The highest PEth concentrations were seen in samples positive for all chronic biomarkers, followed by those also being CDT positive (cut-off 2.0%). All 126 CDTpositive samples were positive for PEth using the lower reporting limit (≥0.05 µmol/l) and for 114 cases (90%) also using the higher limit (>0.30 µmol/l or 210 µg/l). In the CDT-positive cases, the PEth median concentration was 1.71 µmol/l, compared with 0.45 µmol/l for the CDT-negative cases (P < 0.0001). PEth and CDT values were correlated significantly (r = 0.63, P < 0.0001). Among the EtG-positive cases (>1.0 ng/ml), 95% were also PEth positive, and all ethanol-positive cases (>0.10 g/l) were also PEth positive.

Conclusions: For optimal detection of drinking habits, using a combination of short- and longterm alcohol biomarkers provided best information. PEth was the single most positive alcohol biomarker, whereas GGT and MCV offered little additional value over PEth and CDT.

INTRODUCTION

Alcohol consumption is associated with an elevated risk for serious health problems; it affects a large proportion of the population globally and results in significant economic consequences (Rehm et al.,

2018). The health risks are related to the daily amount of alcohol intake (Corrao et al., 2004), and the lower threshold for harmful drinking was recently proposed to be 100 g/week (Wood et al., 2018). WHO has pointed out the implementation of screening for harmful drinking and brief intervention programs as recommended actions, to reduce the burden of excessive alcohol consumption (WHO, 2018).

For screening of harmful alcohol use, alcohol biomarkers are important objective complements to self-reports and structured interviews about drinking habits and can be used in health controls to aid early detection (Hermansson *et al.*, 2010). Other applications of alcohol biomarkers are to monitor compliance in treatment, to monitor drinking during pregnancy and in subjects applying for job, or in regranting of a driving license (Isaksson *et al.*, 2011).

A range of alcohol biomarkers are available based on measurement in blood, urine or hair samples (Niemelä, 2016). A recently introduced biomarker is phosphatidylethanol (PEth) that is measured in whole blood by liquid chromatography-mass spectrometry (LC-MS) methods (Nalesso *et al.*, 2011; Zheng *et al.*, 2011). PEth has demonstrated superior specificity and sensitivity compared with other biomarkers targeting regular high alcohol use ('chronic' biomarkers) (Viel *et al.*, 2012). PEth is formed during ethanol exposure and accumulates over time following repeated and frequent drinking. Each intake of an intoxicating ethanol dose leads to an elevation of the PEth level in whole blood (Schröck *et al.*, 2017). During abstinence, the half-life of PEth differs between individuals in the range 4–10 (median 6) days (Helander *et al.*, 2019a).

PEth has recently been introduced as a routine alcohol biomarker to confirm abstinence or detect harmful drinking (Ulwelling and Smith, 2018). However, an important issue for the latter application is that it appears to be difficult to establish the magnitude of alcohol intake based on a PEth value, as several studies have demonstrated considerable variation in test response between different individuals (Aradottir *et al.*, 2006; Helander *et al.*, 2012, 2019b; Viel *et al.*, 2012; Ulwelling and Smith, 2018). Another important feature that needs additional investigation is the comparison of PEth with other alcohol biomarkers, and how they can best be used in combination. A recent comparison of PEth with other alcohol biomarkers and self-reports in pre- and post-liver transplant patients supported the superior features of PEth (Andresen-Streichert *et al.*, 2017).

The aim of this work was to compare test results for a set of alcohol biomarkers commonly used to indicate recent drinking (called 'acute' biomarkers) or mainly regular high alcohol consumption (called 'chronic' biomarkers) in blood samples received for routine measurement from employment-related health controls.

MATERIALS AND METHODS

Clinical samples

The samples investigated in this study came from patients presenting at Medical Centers at employment agencies and from occupational health units. The subjects typically underwent evaluation concerning risky drinking and were predominantly unemployed. The study included 519 sample sets from 509 patients (80% were men and 8 gave repeated samples). EDTA-whole blood and serum samples taken by venous puncture were received for routine measurement of ethanol, carbohydrate-deficient transferrin (CDT, % disialotransferrin) and gamma-glutamyl transferase (GGT) in serum, and erythrocyte mean corpuscular volume (MCV) in whole blood. Left over aliquots of whole blood were stored at 4°C and used for ethyl glucuronide (EtG) and PEth analysis within 1 week after samples were anonymized.

Analysis of PEth in whole blood

PEth analysis (PEth 16:0/18:1 form) was made by an in-house DIN EN ISO 17025 accredited UPLC-MS/MS method. Twenty

microlitre of whole blood were mixed with 20-ul internal standard (0.142 µmol/l PEth-d₅, Chiron AS, Trondheim, Norway) in isopropanol. To precipitate proteins, 120-ul isopropanol was added followed by mixing and addition of 200-ul n-hexane. After another mixing and centrifugation, the entire supernatant was transferred to new tubes and evaporated to dryness at 45°C for about 10 min with nitrogen. The dry residue was re-dissolved in 200 μ l of a 1 + 4 mix of mobile phase A and B (see below). Following mixing and centrifugation, 10 µl was injected into the UPLC system. Calibration was performed using fortified blank blood at 0.014, 0.043, 0.085, 0.142, 0.356, 0.711, 1.14, 1.42, 3.56 and 7.11 µmol/l PEth 16:0/18:1 using reference material from Avanti Polar Lipids Inc. (Alabaster, AL, USA). For quality controls (QC) at a concentration of 0.05 µmol/l, the CV was 11% and bias 5.0%; at 0.30 µmol/l, the CV was 10.5% and bias 0.2% and at 2.85 µmol/l, the CV was 9.0% and bias 0%. Accuracy in the measurements was confirmed by participation in the EQUALIS AB (Uppsala, Sweden) quality assessment program. The lower quantification limit (LLOQ) was 0.014 µmol/l.

Chromatographic separation was conducted using a Waters Acquity UPLC connected to a Waters Xevo-TQ-S on a BEH C18 column (1.7 μm, 2.1 × 150 mm, Waters) within 3.5 min using gradient elution (mobile phase A = 5 mmol/l ammonium formate in water/isopropanol/acetonitrile (30/10/60; v/v/v), mobile phase B = 5 mmol/l ammonium formate in water/isopropanol/acetonitrile (1/79/20; v/v/v)). The analytical column was kept at 40°C and the flow rate of 0.30 ml/min. Capillary voltage was set to 1.5 kV, the ion source temperature was 150°C and desolvation gas was heated to 650°C and delivered at a flow rate of 800 l/h. Cone gas (N2) was set to 150 l/h, and the collision gas (Ar) was maintained at 0.2 ml/min. The instrument was operated in the ESI negative mode. Three ion transitions (1 quantifier and 2 qualifier ions) for PEth 16:0/18:1 were recorded in SRM mode: m/z 701.4 > 281.2 (quantifier), 701.4 > 255.2, 701.4 > 437.2; PEth-d₅: m/z 706.5 > 281.2(quantifier), 706.5 > 255.1 and 706.5 > 442.2.

Two decision limits were used for PEth: $> 0.050 \, \mu mol/l \, (\sim 35 \, \mu g/l)$ for 'social drinking' and $> 0.30 \, \mu mol/l \, (\sim 210 \, \mu g/l)$ for 'harmful drinking' (Helander and Hansson, 2013).

Analysis of CDT in serum

CDT was determined by a commercial CE- and IVD-marked HPLC method (Chromsystems Instruments & Chemicals GmbH, Gräfelfing, Germany). The decision limit for CDT used to indicate excessive drinking was $\geq 2.0\%$ disialotransferrin (Helander *et al.*, 2017). The CV value for QC samples was 9.3% for Chromsystems CDT-L1 (mean 1.3%; n=21) and 5.4% for CDT-L2 (mean 2.9%; n=21). The accuracy of the method was further confirmed by comparison with the IFCC CDT HPLC reference method (Helander *et al.*, 2017). Baseline integration of transferrin peaks was used according to the recommendation for this decision limit. In six cases, the chromatograms did not allow for the calculation of the CDT value. These cases were excluded from the study but were all indicated to be CDT negative (<2.0%).

Analysis of GGT and MCV and use as combined marker

Measurement of GGT in serum (reference ranges were <1.05 µmol/l·s for males and <0.75 µmol/l·s for females) was made using reagents from Roche Diagnostics, and MCV in whole blood (reference range 85–95 fL) using an instrument from Axon Lab.

A combined GGT/MCV biomarker (both positive) was also used to increase the specificity (Chick *et al.*, 1981; Rosman, 1992).

Analysis of EtG in serum

EtG analysis was made by an in-house DIN EN ISO 17025 accredited UPLC-MS/MS method, which will be reported in detail separately (Neumann et al., 2020). In brief, a 20-µl aliquot of serum was mixed with 200-µl methanol containing 20-pg EtG-d5 (Cerrilliant, Merck KGaA, Darmstadt, Germany). The mixture was shaken thoroughly followed by centrifugation for 10 min at 12,000 × g. After centrifugation, 200 µl of the resulting supernatant was transferred to an autosampler vial and evaporated to dryness using heated nitrogen gas. The residue was redissolved in 80-µl 0.1% formic acid and 10 µl was injected into the UPLC. For QC samples at a concentration of 0.50-ng/ml EtG, the CV was 4.4% and bias 2.2%, and at 3.0 ng/ml, the CV was 3.3% and bias 0.3%. The EtG decision limit was 1.0 ng/ml.

Analysis of ethanol in serum

The serum ethanol concentration was determined using the DRI ethyl alcohol assay from Thermo Fisher Scientific. The QC results for ACQ Science Ethanol 0.50 g/l were mean 0.52, CV 4.4% (n=30); for the 1.30 g/l control mean 1.34, CV 3.4% (n=30) and for the 3.00 g/l control mean 3.04, CV 3.3% (n=38). The ethanol decision limit was 0.10 g/l.

Statistics

Statistical calculations were done using Xact® chart software (Scilab, Hamburg, Germany) and MedCalc (MedCalc Software, Ostend, Belgium).

RESULTS

A large proportion of the 519 blood specimens tested positive for acute (n=294,57%) and chronic (n=359,69%) alcohol biomarkers, demonstrating a high proportion of alcohol drinking in the studied population. PEth in whole blood was the biomarker with overall highest positive rate, with 333 cases (64%) showing a value above the 0.05 µmol/l cut-off (Table 1). PEth was also the only positive chronic biomarker in 100 cases, representing 30% of all PEth-positive cases. For the higher reporting limit indicating 'risky drinking' ($\geq 0.30 \ \mu mol/l$), the number of PEth positives was 238 (46%) and PEth was the only positive chronic biomarker in 38 cases (16%). The distribution of PEth concentrations in all 519 cases is shown in Fig. 1.

Compared with PEth, serum CDT and GGT, whole blood MCV and the GGT/MCV combined biomarker were positive in lower numbers of cases (Table 1). GGT was the only positive chronic biomarker in 26 cases, while in no case, MCV or GGT/MCV was the only positive biomarker. A comparison of the test results for chronic alcohol biomarkers, including the two cut-off limits for PEth, is shown in Fig. 2A and B.

The mean (median) serum ethanol concentration among the 60 positive cases was 1.27 (0.95) g/l, respectively. The other acute alcohol biomarker, EtG in serum, was positive in 294 cases (Table 1), with a mean (median) concentration of 915 (134) ng/ml, respectively. A comparison of the test results for PEth with the two acute alcohol biomarkers is presented in Fig. 2C.

Figure 3 shows the distribution of PEth concentrations in different subgroups from Table 1 and Fig. 2. The highest median concentration was seen in the subgroup being positive for all chronic

Table 1. Overview of positive rates for the different biomarkers alone and for test combinations

Alcohol biomarker	Cut-off	N (%)
PEth in whole blood	≥0.05 µmol/l	333 (64)
PEth in whole blood	≥0.30 µmol/l	238 (46)
CDT in serum	≥2.0%	126 (24)
GGT in serum	>1.05 µmol/l*s (men),	216 (42)
	$> 0.75 \mu mol/l*s$	
	(women)	
MCV in whole blood	>95 fL	136 (41)
GGT and MCV	Both over limits	91 (18)
EtG in serum	\geq 1.0 ng/ml	294 (57)
Ethanol in serum	≥0.10 g/l	60 (12)
Combinations	PEth (≥0.05) N (%)	PEth (≥0.3) N (%)
and CDT	126 (24)	114 (22)
and GGT	190 (37)	172 (33)
and MCV	123 (24)	107 (41)
and GGT and MCV	91 (18)	87 (17)
and EtG	278 (54)	225 (43)
and ethanol	60 (12)	56 (11)

alcohol biomarkers, followed by the subgroup being positive for PEth and CDT.

PEth vs CDT

All 126 cases with a positive CDT test were also positive for PEth using the lower (0.050 μ mol/l) reporting limit, and in 114 cases (90%) using the higher cut-off (\geq 0.30 μ mol/l). In the CDT-positive cases, the mean and median PEth values were 2.07 and 1.71 μ mol/l, respectively, while in the CDT negative cases, the corresponding values were 0.71 and 0.45 μ mol/l (n=207). The Mann–Whitney test for independent samples demonstrated a statistically significant difference between the groups (P < 0.0001).

A regression analysis for PEth vs CDT concentration values showed a significant correlation (r=0.63, P<0.0001). However, there was a large subpopulation of cases (n=114) where CDT was negative but PEth $\geq 0.30~\mu$ mol/l, and a smaller one where CDT was positive but PEth $<0.30~\mu$ mol/l (n=12). In the latter group, the CDT values ranged 2.0–10.1% (median 2.6%) and PEth ranged 0.09–0.28 (median 0.22) μ mol/l.

The mean CDT value in the 186 cases with undetected PEth ($<0.05 \, \mu \text{mol/l}$) was $1.06 \pm 0.29\%$ (SD), while in the subgroup with a negative CDT and a PEth value $\ge 0.30 \, \mu \text{mol/l}$, the mean CDT value was $1.33 \pm 0.35\%$ (n = 114). The difference was statistically significant (Mann–Whitney, P < 0.0001).

PEth vs GGT

Of the 333 PEth-positive cases, 190 (57%) were also positive for GGT (Fig. 2A). The PEth concentrations were significantly higher in the GGT-positive cases than in the 143 negative cases, with mean (median) values of 1.71 (1.26) vs 0.57 (0.26) μ mol/l, respectively (Mann–Whitney, P < 0.0001).

PEth vs MCV

Of the 333 PEth-positive cases, 123 (37%) were positive for MCV. The PEth concentrations were significantly higher in the MCV-positive cases than in the 210 negative cases, with mean (median)

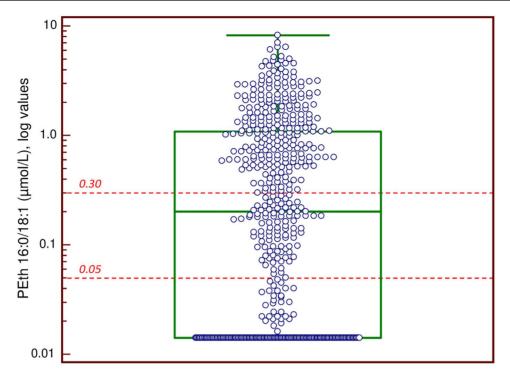


Fig. 1. A plot of all phosphatidylethanol (PEth 16:0/18:1) results presented in log scale (n=519). In 155 cases, the PEth measurement was below the LLOQ (0.014 μ mol/l). The mean value was 0.79 μ mol/l (555 η mol/l), the median value 0.20 μ mol/l (140 η mol/l) and the highest value was 8.17 μ mol/l (5740 η mol/l). The test for normal distribution was negative. The two reporting limits employed (0.30 μ mol/l or \sim 210 μ g/l, and 0.05 μ mol/l or \sim 35 μ g/l, respectively) are indicated (- - -).

values of 1.77 (1.36) vs 0.90 (0.53) μ mol/l, respectively (Mann–Whitney, P < 0.0001).

PEth vs GGT/MCV

Of the 333 PEth-positive cases, 91 (27%) were positive for the GGT/MCV combination (Fig. 2A). The PEth concentrations were significantly higher in the GGT/MCV-positive cases than in the 111 negative cases, with mean (median) values of 2.10 (1.84) vs 0.49 (0.35) μ mol/l, respectively (Mann–Whitney, P < 0.0001).

PEth vs EtG

Of the 294 EtG-positive cases, 278 (95%) were also positive for PEth with a mean (median) concentration of 1.41 \pm 1.38 (1.00) µmol/l (Fig. 4). Of the 225 EtG-negative cases, 55 (24%) were positive for PEth with the mean (median) value of 0.28 \pm 0.34 (0.18) µmol/l.

Of the 333 PEth-positive cases, 278 (83%) were also positive for EtG, the mean (median) concentration being 966 \pm 1826 (178) ng/mL (Fig. 5). Of the 186 PEth-negative cases, 16 (8.6%) were positive for EtG with a mean (median) concentration of 25 ± 46 (6.1) ng/mL. In the 238 cases with a PEth concentration above the upper cut-off (>0.30 μ mol/L), 95% were EtG positive, whereas in the 95 cases with PEth concentrations in the range 0.05–0.30 μ mol/L, 56% were EtG positive.

PEth vs ethanol

Of the 60 cases where ethanol was detected, all tested positive for PEth with a mean (median) concentration of 2.65 \pm 1.78 (2.32) µmol/L (Fig. 4). Of the 333 PEth-positive cases, 18% were also

positive for ethanol (Fig. 2C) and of the 238 cases with a PEth value $> 0.30 \ \mu mol/L$, 25% were positive for ethanol.

T vs GGT/MCVGGT was positive in more than twice as many cases compared with the GGT/MCV test combination (Table 1). In 125 cases being positive for GGT but negative for MCV, high alcohol consumption was not supported by an elevated PEth or CDT in 26 cases (21%). Among these 26, EtG was detected in 5 cases (19%) but ethanol in no one. In 16 cases, the PEth concentrations ranged 0.05–0.30 μ mol/L and EtG was detected in 10 of those (62%), while ethanol was detected in no one. However, in 84 cases high alcohol intake was supported by a positive PEth and/or CDT value. Thus, the addition of MCV as a criterium for a positive GGT test increased test specificity from 80% to 100%, while the sensitivity was reduced to 52%. The PEth concentration difference between the GGT/MCV and GGT positives was statistically different (Mann-Whitney, p=0.013).

Ethanol vs EtG

In all 60 ethanol-positive cases, EtG was also detected in serum with a mean (median) concentration of 3392 ± 2637 (2872) ng/mL. In the 234 ethanol-negative cases containing EtG, the mean (median) value was 280 ± 524 (49) ng/mL (Fig. 5).

DISCUSSION

This study documented a much higher test sensitivity for PEth compared with CDT, GGT and MCV, as indicators of regular high alcohol exposure in subjects undergoing medical investigation at employment agencies and occupational health units. The higher sensitivity of PEth agrees with previous observations (Hartmann *et al.*, 2007;

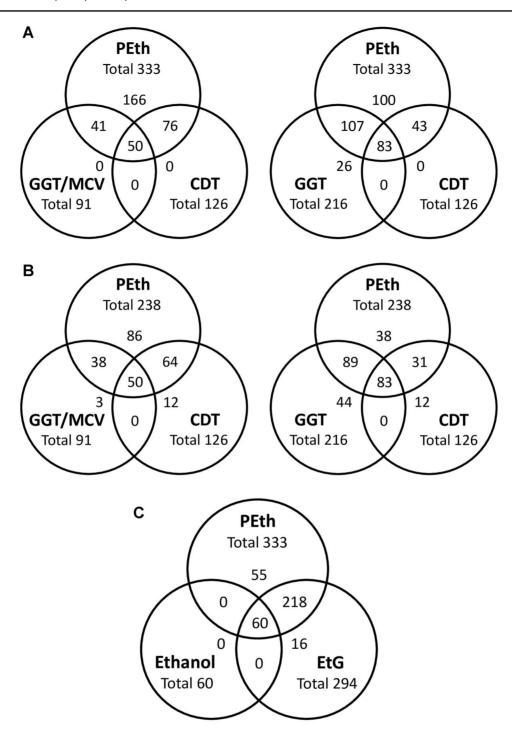


Fig. 2. Comparison of the overlap of positive test results between PEth and other tests used as alcohol biomarkers (CDT (% disialotransferrin); GGT; MCV EtG). The total number of positives for each test is given together with the number in each overlapping category, as well as the number of cases not overlapping. (A and C) Applied PEth reporting limit ≥0.05 μmol/l; (B) applied PEth reporting limit ≥0.30 μmol/l.

Helander et al., 2012; Kechagias et al., 2015; Walther et al., 2015). Most previous studies comparing PEth with CDT involved patients diagnosed with alcohol dependence (Hartmann et al., 2007; Helander et al., 2012; Walther et al., 2015). In two studies, a total of 200 individuals were monitored over time and in both a two-fold higher test-positive rate was seen for PEth (Helander et al., 2012; Walther et al., 2015), similar to the present observations. In a third study, 56 patients were studied while being in detoxification treatment

and, based on the receiver operating characteristic curves, a two-fold higher test sensitivity of PEth over CDT was indicated (Hartmann et al., 2007). In the fourth study, 44 healthy subjects were instructed to drink a fixed amount of red wine daily (33 g/day for men and 16 g/day for women) over a 3-month period (Kechagias et al., 2015). Despite this significant ethanol intake (although not supervised), no subject reached the CDT and PEth cut-offs indicating chronic heavy drinking. However, the statistical analysis demonstrated better

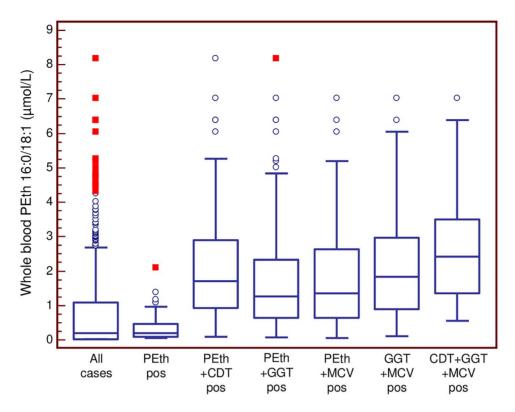


Fig. 3. PEth concentrations in cases above 0.05 µmol/l in categories from Fig. 2A. Results are Box-and-whisker plots, where the box represents the 25–75 percentile, the middle line the median, the vertical lines extend to minimum and maximum values, with the exception of statistically 'outside' (open circle) and 'far out' (filled square) values.

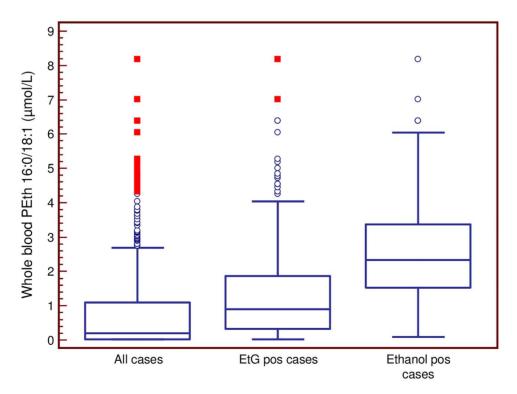


Fig. 4. PEth concentrations in cases above 0.05 µmol/l in categories from Fig. 2C. Results are Box-and-whisker plots, where the box represents the 25–75 percentile, the middle line the median, the vertical lines extend to minimum and maximum values, with the exception of statistically 'outside' (open circle) and 'far out' (filled square) values.

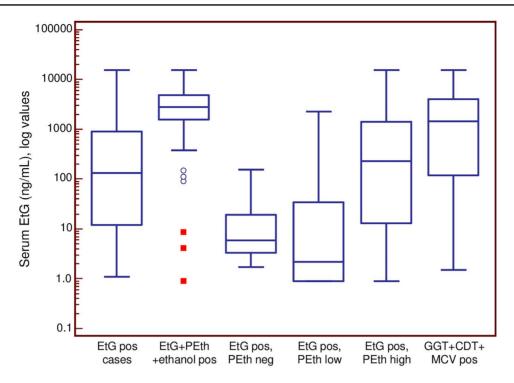


Fig. 5. EtG concentrations in cases with different combinations of positive results for PEth and ethanol. Results are Box-and-whisker plots, where the box represents the 25–75 percentile, the middle line the median, the vertical lines extend to minimum and maximum values, with the exception of statistically 'outside' (open circle) and 'far out' (filled square) values.

performance of PEth in discrimination between the study group and the control group.

An interesting detail from the present study is the observation of 12 cases where CDT was positive but PEth was below the 0.30 µmol/L cut-off used to indicate 'heavy drinking', which was contrary to the expected higher test sensitivity of PEth. This could indicate that in some individuals PEth formation in response to alcohol intake is relatively low (Helander *et al.*, 2012), or the result of the slower elimination rate of CDT after stopping drinking alcohol. Nevertheless, in all 12 cases, PEth was detected and when using the interpretation guideline proposed by Ulwelling and Smith (2018), all 12 cases would be classified as 'significant consumption'.

Reference cut-offs for interpreting PEth concentrations are not firmly established. When the PEth 16:0/18:1 homologue was first used as the single target analyte instead of the sum of all PEth forms, a cut-off concentration of 0.20 µmol/L for heavy drinking was proposed (Zheng et al., 2011). Following a national harmonization of PEth testing in Sweden, the cut-off was later increased to > 0.30 µmol/L (~210 µg/L) to increase test specificity and applied as a generally accepted cut-off to indicate heavy drinking, whereas $> 0.05 \mu \text{mol/L}$ ($\sim 35 \mu \text{g/L}$) was applied as a lower limit to indicate 'social drinking' (Helander and Hansson, 2013). Recently, Ulwelling and Smith (2018) have proposed 20-200 ng/mL (i.e. ~ 0.03 -0.30 µmol/L) to indicate 'significant consumption' and > 200 ng/mL for 'heavy consumption' and Kummer et al. (2016) have also favored a similar cut-off (221 ng/mL) for chronic excessive drinking. A recent study from our group also supported the use of 0.30 µmol/L as the cut-off to indicate harmful drinking (>50 g/day) (Helander et al., 2019). This limit is to be considered as safe and allows the interpretation of chronic high alcohol intake even when considering

the inter-individual variability in PEth response to alcohol exposure (Helander *et al.*, 2019b).

The CDT test is targeting long-term heavy alcohol consumption, but it is less sensitive than PEth for detecting harmful drinking. This is partly a consequence of the applied CDT cut-off limit of 2.0% recommended for HPLC methods, which is based on the mean + 3SD for controls to increase test specificity (Helander et al., 2017). The subgroup of cases with a PEth concentration $> 0.30 \mu \text{mol/L}$ but a CDT value below 2.0% had significantly higher CDT values than the subgroup with a PEth concentration $< 0.30 \mu \text{mol/L}$ (mean 1.35 vs 1.10%, P < 0.0001). This demonstrated that there was indeed a response with increased CDT levels in this PEth positive group. Based on the CDT results for the PEth-negative group, a higher cut-off of 1.9% can be calculated using the mean + 3SD, supporting the recommended cut-off of $\geq 2.0\%$ for a positive CDT test (Helander et al., 2017).

GGT is a liver function test that is not specific for use as an alcohol biomarker but rather relates to liver damage that may or may not be cause by chronic heavy drinking, while MCV has the feature of high specificity but low sensitivity (Helander and Jones, 2006). In the present study, the use of the GGT/MCV test combination increased the selectivity to 100% but decreased the sensitivity by almost 50%. The observed low sensitivity agrees with previous observations (Chick *et al.*, 1981; Rosman, 1992). Since the PEth and CDT tests covered all cases that were positive by GGT and GGT/MCV, it indicates a very limited value of these tests when PEth and CDT are available. However, GGT may have value as an additional test to reveal alcohol-related liver damage.

An interesting observation was that all cases with a detectable ethanol concentration in blood when visiting the medical units had PEth concentrations above the higher cut-off indicating 'risky drinking'. For the EtG-positive cases, demonstrating recent alcohol intake but not necessarily being under the influence, there was an association with elevated PEth concentrations. Also the fraction of EtG-positive samples increased with elevated PEth concentrations, from 9% to 95%. The combined use of short- ('acute') and long-term ('chronic') alcohol biomarkers provide a more complete information regarding drinking habits as noted before (Helander *et al.*, 2012). EtG is usually used as a urinary alcohol biomarker and as a complement to drug testing based on immunoassay screening (Böttcher *et al.*, 2008). This study instead employed EtG measurement in serum by an LC-MS/MS method with a 100-fold lower measuring range. This opens for the possibility to measure both PEth and EtG in the same collected blood sample. EtG measurements might help to differentiate between currently abstinent and drinking patients.

In conclusion, this study confirms the high sensitivity of PEth as a biomarker for alcohol exposure. The inborn high specificity, being an ethanol metabolite, also favors use of this biomarker, although it is not possible to determine the exact amount of alcohol consumed from the test value. GGT and MCV, which have traditionally been employed as alcohol biomarkers, appear to have no additional value over PEth and CDT for detection of chronic high alcohol intake. For optimal detection of harmful drinking in clinical and forensic settings, a combination of short- and long-term alcohol biomarkers covering different amounts of consumption appears to provide the best information regarding individual drinking habits.

REFERENCES

- Andresen-Streichert H, Beres Y, Weinmann W et al. (2017) Improved detection of alcohol consumption using the novel marker phosphatidylethanol in the transplant setting: results of a prospective study. *Transpl Int* 30:611–20.
- Aradottir S, Asanovska G, Gjerss S et al. (2006) Phosphatidylethanol (PEth) concentrations in blood are correlated to reported alcohol intake in alcohol-dependent patients. Alcohol Alcohol 41:431–7.
- Böttcher M, Beck O, Helander A (2008) Evaluation of a new immunoassay for urinary ethyl glucuronide testing. *Alcohol Alcohol* 43:46–8.
- Chick J, Kreitman N, Plant M (1981) Mean cell volume and gammaglutamyl-transpeptidase as markers of drinking in working men. *Lancet* 317:1249–51.
- Corrao G, Bagnardi V, Zambon A et al. (2004) A meta-analysis of alcohol consumption and risk for 15 diseases. Prev Med 38:613–9.
- Hartmann S, Aradottir S, Graf M et al. (2007) Phosphatidylethanol as a sensitive and specific biomarker: comparison with gamma-glutamyl transpeptidase, mean corpuscular volume and carbohydrate-deficient transferrin. Addict Biol 12:81–4.
- Helander A, Böttcher M, Dahmen N et al. (2019a) Elimination characteristics of the alcohol biomarker phosphatidylethanol (PEth) in blood during alcohol detoxification. Alcohol Alcohol 54:251–7.
- Helander A, Hansson T (2013) National harmonization of the alcohol biomarker PEth. *Lakartidningen* 110:1747–8.
- Helander A, Hermansson U, Beck O (2019b) Dose-response characteristics of the AlcoholBiomarker Phosphatidylethanol (PEth)—a study of outpatients in treatment for reduced drinking. *Alcohol Alcohol* **54**:567–73.
- Helander A, Jones AW (2006) Recent advances in biochemical tests for acute and chronic biomarkers of alcohol consumption. In Karch SB (ed). *Drug Abuse Handbook*. Boca Raton, FL, USA: CRC Press, 402–27.

- Helander A, Péter O, Zheng Y (2012) Monitoring of the alcohol biomarkers PEth, CDT and EtG/EtS in an outpatient treatment setting. Alcohol Alcohol 47:552–7.
- Helander A, Wielders J, Anton R et al. (2017) Standardisation and use of the alcohol biomarker carbohydrate-deficient transferrin (CDT). Clin Chim Acta 467:15–20.
- Hermansson U, Helander A, Brandt L et al. (2010) Screening and brief intervention for risky alcohol consumption in the workplace: results of a 1-year randomized controlled study. Alcohol Alcohol 45:252–7.
- Isaksson A, Walther L, Hansson T et al. (2011) Phosphatidylethanol in blood (B-PEth): a marker for alcohol use and abuse. Drug Test Anal 3: 195–200
- Kechagias S, Dernroth DN, Blomgren A et al. (2015) Phosphatidylethanol compared with other blood tests as a biomarker of moderate alcohol consumption in healthy volunteers: a prospective randomized study. Alcohol Alcohol 50:399–406.
- Kummer N, Ingels AS, Wille SM et al. (2016) Quantification of phosphatidylethanol 16:0/18:1, 18:1/18:1, and 16:0/16:0 in venous blood and venous and capillary dried blood spots from patients in alcohol withdrawal and control volunteers. Anal Bioanal Chem 408: 825–38
- Nalesso A, Viel G, Cecchetto G et al. (2011) Quantitative profiling of phosphatidylethanol molecular species in human blood by liquid chromatography high resolution mass spectrometry. J Chromatogr A 1218: 8423–31.
- Neumann J, Beck O, Helander A *et al.* (2020) Sensitive determination of ethyl glucuronide in serum and whole blood: detection time after alcohol exposure compared with urine. *J Lab Med* (submitted for publication).
- Niemelä O (2016) Biomarker-based approaches for assessing alcohol use disorders. Int J Environ Res Public Health 13:166.
- Rehm J, Mathers C, Popova S et al. (2018) Global burden of disease and injury and economic cost attributed to alcohol use and alcohol-use disorders. Lancet 373:2223–33.
- Rosman AS (1992) Utility and evaluation of biochemical markers of alcohol consumption. *J Subst Abuse* 4:277–97.
- Schröck A, Thierauf-Emberger A, Schürch S *et al.* (2017) Phosphatidylethanol (PEth) detected in blood for 3 to 12 days after single consumption of alcohol a drinking study with 16 volunteers. *Int J Leg Med* 131: 153–60.
- Ulwelling W, Smith K (2018) The PEth blood test in the security environment: what it is; why it is important; and interpretative guidelines. *J Forensic Sci* 63:1634–40.
- Viel G, Boscolo-Berto R, Cecchetto G et al. (2012) Phosphatidylethanol in blood as a marker of chronic alcohol use: a systematic review and metaanalysis. Int J Mol Sci 13:14788–812.
- Walther L, de Bejczy A, Löf E *et al.* (2015) Phosphatidylethanol is superior to carbohydrate-deficient transferrin and γ-glutamyltransferase as an alcohol marker and is a reliable estimate of alcohol consumption level. *Alcohol Clin Exp Res* 39:2200–8.
- WHO (2018) Alcohol ways to reduce the burden from harmful use of alcohol. www.who.int/news-room/fact-sheets/detail/alcohol (February 2019, date last accessed).
- Wood AM, Kaptoge S, Butterworth AS et al. (2018) Risk thresholds for alcohol consumption: combined analysis of individual-participant data for 599 912 current drinkers in 83 prospective studies. Lancet 391: 1513–23.
- Zheng Y, Beck O, Helander A (2011) Method development for routine liquid chromatography-mass spectrometry measurement of the alcohol biomarker phosphatidylethanol (PEth) in blood. Clin Chim Acta 412:1428–35.